



Europäisches  
Patentamt

European  
Patent Office

Office européen  
des brevets

4/1  
618  
GB 00/02485

PCT/GB 00/02485  
0/018783 #2

4

Bescheinigung

Certificate

Attestation

REC'D 25 OCT 2000

WIPO

PCT

Die angehefteten Unterla-  
gen stimmen mit der  
ursprünglich eingereichten  
Fassung der auf dem näch-  
sten Blatt bezeichneten  
europäischen Patentanmel-  
dung überein.

The attached documents  
are exact copies of the  
European patent application  
described on the following  
page, as originally filed.

Les documents fixés à  
cette attestation sont  
conformes à la version  
initialement déposée de  
la demande de brevet  
européen spécifiée à la  
page suivante.

Patentanmeldung Nr. Patent application No. Demande de brevet n°

99304975.8

**PRIORITY  
DOCUMENT**  
SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH RULE 17.1(a) OR (b)

Der Präsident des Europäischen Patentamts;  
Im Auftrag

For the President of the European Patent Office

Le Président de l'Office européen des brevets  
p.o.

I.L.C. HATTEN-HECKMAN

DEN HAAG, DEN  
THE HAGUE, 23/10/00  
LA HAYE, LE

**THIS PAGE BLANK (USPTO)**



Europäisches  
Patentamt

European  
Patent Office

Office européen  
des brevets

**Blatt 2 der Bescheinigung  
Sheet 2 of the certificate  
Page 2 de l'attestation**

Anmeldung Nr.:  
Application no.:  
Demande n°: **99304975.8**

Anmeldetag:  
Date of filing: **24/06/99**  
Date de dépôt:

Anmelder:  
Applicant(s):  
Demandeur(s):  
**BIOCOMPATIBLES LIMITED**  
**Farnham, Surrey GU9 8QL**  
**UNITED KINGDOM**

Bezeichnung der Erfindung:  
Title of the invention:  
Titre de l'invention:  
**Balloon expandable stent**

In Anspruch genommene Priorität(en) / Priority(ies) claimed / Priorité(s) revendiquée(s)

Staat:  
State:  
Pays:

Tag:  
Date:  
Date:

Aktenzeichen:  
File no.  
Numéro de dépôt:

Internationale Patentklassifikation:  
International Patent classification:  
Classification internationale des brevets:

**A61F2/06**

Am Anmeldetag benannte Vertragsstaaten:  
Contracting states designated at date of filing: **AT/BE/CH/CY/DE/DK/ES/FI/FR/GB/GR/IE/IT/LI/LU/MC/NL/PT/SE**  
Etats contractants désignés lors du dépôt:

Bemerkungen:  
Remarks:  
Remarques:

**THIS PAGE BLANK (USPTO)**

**Balloon Expandable Stent**

The present invention relates to balloon expandable stents for delivering into body lumens, in particular to stents formed from tubes, especially metal tubes. In particular this invention relates to means for retaining the stent on the balloon during storage and delivery of the stent through the body lumen prior to deployment, without adversely affecting the balloon strength or deployment of the stent.

Balloon expandable stent, either made from wires, or made from metal tubes which are cut or etched to form openings in the surface are crimped onto the balloon delivery device either as part of the manufacturing/assembly process, or immediately prior to use by a surgeon. Generally the stent is positioned over the balloon, sometimes on a sleeve which is positioned over the balloon, and is then crimped down onto the balloon. During the delivery procedure, when the delivery catheter carrying the stent is being maneuvered through body lumens, the stent is subjected to forces which may dislodge the stent from its desired position on the balloon.

Means have been described for retaining the stent in position on the balloon during delivery. For instance protrusions have been provided on the balloon, or the catheter near to the balloon, having shoulders above and/or below the stent location which bear against the stent when it is subjected to an axial force. Alternatively protrusions may be provided on the external surface of the balloon, or on a sleeve located between the stent and the balloon, which protrude into the holes through the wall of the stent. Again these protrusions have shoulders which may bear against the axially directed surfaces of those holes. However the procedures used to make such balloons tend to lead to weakening of the balloon wall and/or increase in the pressure required to inflate the balloon and/or require additional manufacturing steps and steps for careful positioning of the stent upon the balloon.

Other methods have involved the application of an adhesive layer between the stent and the balloon. However such layers may have an

adverse effect on balloon strength and/or inflation characteristics. Furthermore it is difficult to ensure a good interfacial contact between the stent and the adhesive and/or adhesive and balloon. Such adhesives may also have an adverse effect on biocompatibility.

5           Other solutions to this problem have involved providing an external sheath surrounding the balloon when mounted on the catheter which must be retracted prior to deployment of the stent. This involves an extra step in the delivery process, increases the external diameter of the stent/delivery device combination and increases the likelihood of mechanical failure of the  
10       delivery device.

          The present invention seeks to solve the above problems. Some embodiments of the invention also improve the biocompatibility of the delivery device, and stent once delivered. Some embodiments of the invention may also provide improved lubricity of the delivery device during  
15       the stent delivery procedure.

          According to the invention there is provided a new kit comprising a balloon catheter comprising a balloon at or near its distal end, and a stent mounted on the balloon, characterized in that in that the exterior surface of the balloon and stent are provided with a coherent coating comprising a film-  
20       forming polymer.

          In the invention the coating is preferably continuous around the exterior surface of the balloon/stent, over at least a portion of the axial extent of that section. Preferably the coating is provided along the entire axial length of the stent, most preferably being continuous around the  
25       circumference throughout the axial length. Preferably the coating extends beyond at least the distal stent end and preferably also the proximal stent end. It may extend along the exterior surface of the balloon catheter shaft proximal of the balloon.

          The coating may comprise components other than the film forming  
30       polymer, for instance fillers, diluents, plasticisers, colouring agents, opacifying agents, pharmaceutically active agents, radioactive or other

imaging agents etc. Often, however, the coating may consist essentially only of the film forming polymer.

The film forming polymer is preferably crosslinked to provide adequate coherent strength. Preferably the crosslinking of the polymer is achieved wholly or mainly after coating of the polymer on the surface which will be described in more detail in connection with the process below.

Preferably the polymer is biocompatible. Since the stent is primarily used in vascular lumens, the coating is preferably additionally hemo-compatible. The bio/hemo-compatibility should preferably persist during the delivery process and, preferably also, after the delivery process. Where the coating is biostable, that is not degraded after deployment of the device, the biocompatibility of the coating should persist throughout the period during which the coating remains on the stent surface after deployment.

The biocompatibility is preferably achieved by the use of a polymer having pendent zwitterionic groups. Preferably a polymer having zwitterionic moieties is formed from radical polymerization of ethylenically unsaturated monomers including a zwitterionic monomer.

Preferably the zwitterionic monomer has the general formula I:



YBX

wherein

B is a straight or branched alkylene (alkanediyl), alkyleneoxaalkylene or alkylene oligo-oxaalkylene chain optionally containing one or more fluorine atoms up to and including perfluorinated chains or, if X or Y contains a terminal carbon atom bonded to B, a valence bond;


X is a zwitterionic group; and

Y is an ethylenically unsaturated polymerisable group selected from



$\text{CH}_2=\text{C}(\text{R})-\text{CH}_2-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R})-\text{CH}_2\text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R})\text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R})-\text{O}-$ ,  
 $\text{CH}_2=\text{C}(\text{R})\text{CH}_2\text{OC}(\text{O})\text{N}(\text{R}^1)-$ ,  $\text{R}^2\text{OCCCR}=\text{CRC}(\text{O})-\text{O}-$ ,  $\text{RCH}=\text{CHC}(\text{O})\text{O}-$ ,  
 $\text{RCH}=\text{C}(\text{COOR}^2)\text{CH}_2-\text{C}(\text{O})-\text{O}-$ ,

5

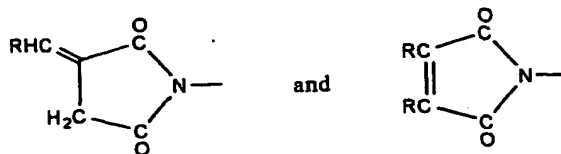

wherein:

R is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group;

10  $\text{R}^1$  is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group or  $\text{R}^1$  is  $-\text{B}-\text{X}$  where B and X are as defined above; and

$\text{R}^2$  is hydrogen or a  $\text{C}_{1-4}$  alkyl group;


A is  $-\text{O}-$  or  $-\text{NR}^1-$ ;

15 K is a group  $-(\text{CH}_2)_p\text{OC}(\text{O})-$ ,  $-(\text{CH}_2)_p\text{C}(\text{O})\text{O}-$ ,  
 $-(\text{CH}_2)_p\text{OC}(\text{O})\text{O}-$ ,  $-(\text{CH}_2)_p\text{NR}^3-$ ,  $-(\text{CH}_2)_p\text{NR}^3\text{C}(\text{O})-$ ,  
 $-(\text{CH}_2)_p\text{C}(\text{O})\text{NR}^3-$ ,  $-(\text{CH}_2)_p\text{NR}^3\text{C}(\text{O})\text{O}-$ ,  $-(\text{CH}_2)_p\text{OC}(\text{O})\text{NR}^3-$ ,  
 $-(\text{CH}_2)_p\text{NR}^3\text{C}(\text{O})\text{NR}^3-$  (in which the groups  $\text{R}^3$  are the same or different),  
 $-(\text{CH}_2)_p\text{O}-$ ,  $-(\text{CH}_2)_p\text{SO}_3-$ , or, optionally in combination with B, a valence bond  
 p is from 1 to 12; and

20  $\text{R}^3$  is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group.

In the zwitterionic monomer the general formula I, the zwitterionic group preferably has the general formula III

25



III

in which the moieties  $\text{A}^2$  and  $\text{A}^3$ , which are the same or different, are  $-\text{O}-$ ,  $-\text{S}-$ ,  $-\text{NH}-$  or a valence bond, preferably  $-\text{O}-$ , and  $\text{W}^+$  is a group  
 30 comprising an ammonium, phosphonium or sulphonium cationic group and a group linking the anionic and cationic moieties which is preferably a  $\text{C}_{1-12}$ -alkanediyl group,

preferably in which  $\text{W}^+$  is a group of formula

$-W^1-N^+R^9_3$ ,  $-W^1-P^+R^{10}_3$ ,  $-W^1-S^+R^{10}_2$  or  $-W^1-Het^+$  in which:


$W^1$  is alkanediyl of 1 or more, preferably 2-6 carbon atoms optionally containing one or more ethylenically unsaturated double or triple bonds, disubstituted-aryl (arylene), alkylene arylene, arylene alkylene, or alkylene  
 5 aryl alkylene, cycloalkanediyl, alkylene cycloalkyl, cycloalkyl alkylene or alkylene cycloalkyl alkylene, which group  $W^1$  optionally contains one or more fluorine substituents and/or one or more functional groups; and

either the groups  $R^9$  are the same or different and each is hydrogen or alkyl of 1 to 4 carbon atoms, preferably methyl, or aryl, such as phenyl, or  
 10 two of the groups  $R^9$  together with the nitrogen atom to which they are attached form an aliphatic heterocyclic ring containing from 5 to 7 atoms, or the three groups  $R^9$  together with the nitrogen atom to which they are attached form a fused ring structure containing from 5 to 7 atoms in each ring, and optionally one or more of the groups  $R^9$  is substituted by a  
 15 hydrophilic functional group, and

the groups  $R^{10}$  are the same or different and each is  $R^9$  or a group  $OR^9$ , where  $R^9$  is as defined above; or

Het is an aromatic nitrogen-, phosphorus- or sulphur-, preferably nitrogen-, containing ring, for example pyridine.


20 Most preferably, the zwitterionic group of the formula III, has the general formula IV:

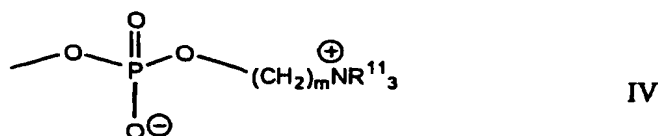

25 where the groups  $R^{11}$  are the same or different and each is hydrogen or  $C_{1-4}$  alkyl, and  $m$  is from 1 to 4, in which preferably the groups  $R^{11}$  are the same preferably methyl.

Alternatively, the zwitterionic group may be a betaine group (ie in  
 30 which the cation is closer to the backbone), for instance a sulfo-, carboxy- or phospho-betaine. A betaine group should have no overall charge and is preferably therefore a carboxy- or sulfo-betaine. If it is a phosphobetaine

the phosphate terminal group must be a diester, i.e., be esterified with an alcohol. Such groups may be represented by the general formula V



5

in which  $A^4$  is a valence bond, -O-, -S- or -NH-, preferably -O-;

V is a carboxylate, sulphonate or phosphate diester (monovalently charged) anion;


10  $R^{12}$  is a valence bond (together with  $A^4$ ) or alkanediyl, -C(O)alkylene- or -C(O)NHalkylene preferably alkanediyl, and preferably containing from 1 to 6 carbon atoms in the alkanediyl chain;

the groups  $R^{13}$  are the same or different and each is hydrogen or alkyl of 1 to 4 carbon atoms or the groups  $R^{13}$  together with the nitrogen to which they are attached form a heterocyclic ring of 5 to 7 atoms; and

15  $R^{14}$  is alkanediyl of 1 to 20, preferably 1 to 10, more preferably 1 to 6 carbon atoms.

One preferred sulphobetaine monomer has the formula VI

20

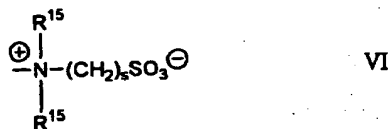


25 where the groups  $R^{15}$  are the same or different and each is hydrogen or  $C_{1-4}$  alkyl and s is from 2 to 4.

Preferably the groups  $R^{15}$  are the same. It is also preferable that at least one of the groups  $R^{15}$  is methyl, and more preferable that the groups  $R^{15}$  are both methyl.

Preferably s is 2 or 3, more preferably 3.

30

Alternatively the zwitterionic group may be an amino acid moiety in which the alpha carbon atom (to which an amine group and the carboxylic acid group are attached) is joined through a linker group to the backbone of the biocompatible polymer. Such groups may be represented by the general formula VII

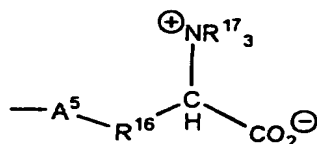

VII

- 5 in which  $\text{A}^5$  is a valence bond, -O-, -S- or -NH-, preferably -O-,  
 $\text{R}^{16}$  is a valence bond (optionally together with  $\text{A}^5$ ) or alkanediyl, -C(O)alkylene- or -C(O)NHalkylene, preferably alkanediyl and preferably containing from 1 to 6 carbon atoms; and

- the groups  $\text{R}^{17}$  are the same or different and each is hydrogen or alkyl  
 10 of 1 to 4 carbon atoms, preferably methyl, or two or three of the groups  $\text{R}^{17}$ , together with the nitrogen to which they are attached, form a heterocyclic ring of from 5 to 7 atoms, or the three group  $\text{R}^{17}$  together with the nitrogen atom to which they are attached form a fused ring heterocyclic structure containing from 5 to 7 atoms in each ring.



- 15 Preferably the monomers used to form the polymer include a surface binding monomer having the general formula II



II


wherein  $\text{Y}^1$  is selected from

20




- 25  $\text{CH}_2=\text{C}(\text{R}^5)-\text{CH}_2-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^5)-\text{CH}_2\text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R}^5)\text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R}^5)-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^5)\text{CH}_2\text{OC}(\text{O})\text{N}(\text{R}^6)-$ ,  $\text{R}^7\text{OOC}\text{C}\text{R}^5=\text{C}\text{R}^5\text{C}(\text{O})-\text{O}-$ ,  
 $\text{R}^5\text{CH}=\text{CHC}(\text{O})\text{O}-$ ,  $\text{R}^5\text{CH}=\text{C}(\text{COOR}^7)\text{CH}_2-\text{C}(\text{O})-\text{O}-$ ,

30



and



wherein:

$R^5$  is hydrogen or a  $C_1$ - $C_4$  alkyl group;

$R^6$  is hydrogen or a  $C_1$ - $C_4$  alkyl group or  $R^6$  is  $R^4$ ;

$R^7$  is hydrogen or a  $C_{1-4}$  alkyl group;

$A^1$  is  $-O-$  or  $-NR^6-$ ; and

5  $K^1$  is a group  $-(CH_2)_qOC(O)-$ ,  $-(CH_2)_qC(O)O-$ ,  
 $-(CH_2)_qOC(O)O-$ ,  $-(CH_2)_qNR^8-$ ,  $-(CH_2)_qNR^8C(O)-$ ,  
 $-(CH_2)_qC(O)NR^8-$ ,  $-(CH_2)_qNR^8C(O)O-$ ,  $-(CH_2)_qOC(O)NR^8-$ ,  
 $-(CH_2)_qNR^8C(O)NR^8-$  (in which the groups  $R^8$  are the same or different),  
 $-(CH_2)_qO-$ ,  $-(CH_2)_qSO_3-$ , or a valence bond

10  $q$  is from 1 to 12;

and  $R^8$  is hydrogen or a  $C_1$ - $C_4$  alkyl group;

and  $R^4$  is a surface binding group, selected from hydrophobic groups,  
 ionic groups, reactive groups capable of forming covalent bonds with surface  
 functional groups on the surface of the tube and crosslinkable groups  
 15 capable of forming intermolecular crosslinks, optionally in conjunction with  
 curing agents.

In the binding monomer of the general formula II, the group  $R^4$  is  
 preferably

- a) a straight or branched alkyl, alkoxyalkyl or oligoalkoxyalkyl  
 20 chain containing 6 or more, preferably 6 to 24 carbon atoms, unsubstituted  
 or substituted by one or more fluorine atoms optionally containing one or  
 more carbon carbon double or triple bonds; or
- b) a siloxane group  $-(CR^{18a})_2)_{qq}(SiR^{19})_2)_{pp}R^{19}$  in which each  
 group  $R^{18}$  is the same or different and is hydrogen or alkyl of 1 to 4 carbon  
 25 atoms, or aralkyl, for example benzyl or phenethyl, each group  $R^{19}$  is alkyl of  
 1 to 4 carbon atoms,  $qq$  is from 1 to 6 and  $pp$  is from 0 to 49; or
- c) a crosslinkable group, capable of reacting with the groups of  
 the same definition, or with groups of a different definition provided by a  
 mixture of monomers of the general formula II, having different groups  $R^4$ .

30 Preferred crosslinkable groups have the formula  $-R^{20}Q$ , where

$R^{20}$  is a valence bond or, more preferably, a straight or branched  
 alkanediyl, alkyleneoxyalkylene or alkylene(oligooxyalkylene) group and

Q is a reactive group selected from cinnamyl, epoxy,  $-\text{CHOHCH}_2\text{Hal}$  (in which Hal is a halogen atom), methylol, silyl and siloxyl groups containing one or more reactive substituents such as halogen, for example chlorine, or alkoxy, generally containing from 1 to 4 carbon atoms, for example methoxy or ethoxy, hydroxyl, amino, carboxyl, ethylenically acetylenically unsaturated crosslinkable groups, acetoacetoxyl, chloroalkylsulphone, succinimido, tosylate, triflate, imidazolecarbonylamino or optionally substituted triazine groups.

Most preferred definitions of  $\text{R}^4$  are  $\text{C}_{6-18}$ -alkyl, -alkenyl or -alkynyl, optionally including fluorine substituents, and mixtures of different groups -  $\text{R}^{20}\text{-Q}$ , in which the groups  $\text{R}^{20}$  are the same or different and each represent  $\text{C}_{2-6}$ -alkanediyl, and one of the groups Q is hydroxyl and the other is a reactive silyl group, preferably having the formula  $\text{Si}(\text{OR}^{22})_3$ , where each group  $\text{R}^{22}$  is  $\text{C}_{1-4}$ -alkyl, preferably methyl or ethyl and n is 0 or 1. A suitable mixture of two comonomers of the formula II is of hydroxyalkylmethacrylate and trimethoxysilylalkyl methacrylate, preferably in which both alkanediyl groups  $\text{R}^{20}$  are the same and are, most preferably, propyl. Preferably the monomers include hydrophobic surface binding group containing monomers and cross-linkable group containing monomers.

In monomers of the formula I and II, Y and  $\text{Y}^1$  are preferably  $\text{H}_2\text{C}=\text{C}(\text{R})\text{C}(\text{O})\text{A}-$  and  $\text{H}_2\text{C}=\text{C}(\text{R}^5)\text{C}(\text{O})\text{A}^1-$ , respectively. R and  $\text{R}^5$  are preferably hydrogen or, more preferably, methyl. A and  $\text{A}^1$  are preferably the same and are most preferably -O-.

B is preferably  $\text{C}_{2-18}$ , more preferably  $\text{C}_{2-6}$ -alkanediyl, branched, or, preferably, straight chain, that is  $(\text{CH}_2)_r$ , where r is 2 to 18, preferably 2 to 6.

The ethylenically unsaturated monomers may include diluent monomers, for instance which may be added to adjust the solubility of the polymer in the coating composition from which it is coated, to adjust the hydrophilicity/phobicity, to control the flexibility of the coating, or for other reasons. Such monomers are generally non-ionic. Suitable diluent monomers are alkyl(alk)acrylates, for instance having 1 to 4 carbon atoms in the alkyl group, N-alkyl- or N,N-dialkyl(alk)acrylamides, for instance having 1

to 4 carbon atoms in the or each alkyl group, (alk)acrylamide, hydroxylalkyl(alk)acrylates, for instance having 1 to 6 carbon atoms in the alkyl group, vinyl lactams, such as vinylpyrrolidone, and styrene. Mixtures may be used.

5           The ethylenically unsaturated monomers from which the polymer having zwitterionic moieties is formed may include other functional monomers. For instance monomers having functional groups may provide attachment points for ligands such as pharmaceutically active agents, specific binding moieties, or antithrombogenic agents. Comonomers may  
10           alternatively include ionic groups, for instance for providing electrostatic attraction with counterionically charged moieties desired to be bonded to the coating. For instance cationic or cationisable monomers may allow loading of the zwitterionic polymer coating of the graft by anionically charged mucopolysaccharides such as heparin, which may reduce thrombogenicity of  
15           the graft still further.

          Preferably the zwitterionic monomer is used in the monomer mixture in a molar proportion of at least 1%, preferably less than 75%, more preferably in the range 5 to 50%, most preferably 10-33%. The surface binding monomer is generally used in molar proportion of at least 2%,  
20           preferably at least 5% or at least 10%, more preferably in the range 15 to 99%. Where the surface binding monomers provide cross-linkability, the level of reactive cross-linkable groups is preferably in the range 5 to 33%. Where the surface binding monomer comprises hydrophobic physisorbable groups, it is preferably present in a molar amount in the range 50 to 99%,  
25           more preferably 60-95%.

          In a particularly preferred embodiment of the invention the polymer used is as described in our co-pending application publication number WO-A-98/30615.

          Where the polymer is formed from monomer including reactive groups  
30           Q, in the kit of the invention, such groups have been reacted to provide covalent bonds to the underlying surface functional groups, and/or intermolecular and intramolecular crosslinking. It is particularly preferred in

the invention that the monomers include crosslinkable groups Q and the in the novel kit, the polymer has been subjected to conditions whereby crosslinking has taken place. Crosslinking improves the coherent strength of the coating and hence the retention of the stent on the balloon.

5 The kit of the invention should be sterile or sterilizable. The kit may be provided in a closed package, and is preferably sterile within the package. Whilst sterilization maybe achievable by sterilizing the individual components, or by sterilizing the partially assembled device, for instance the balloon catheter/stent combination and, separately, the coating composition,  
10 preferably the coated kit is subjected to sterilization.

Sterilization maybe by subjecting the device to high temperature and pressures, for instance in an autoclave, by exposure to irradiation, or preferably, by treatment with ethylene oxide gas.

The present inventors have found that exposure of certain useful  
15 polymers to ethylene oxide gas may result in improvement in the function of the polymer to retain the stent on the balloon. Thus when the polymer having the preferred groups Q comprising reactive silyl groups of the formula  $\text{Si}(\text{OR}^{22})_3$ , contacting the polymer with ethylene oxide, before, during, after or instead of subjecting the polymer to any other crosslinking conditions, result  
20 in improved stent retention.

It is believed that polymers having pendent reactive silyl groups of the formula  $\text{Si}(\text{OR}^{22})_3$  have not previously been contacted with gaseous ethylene oxide to provide curing of the polymer. According to a second aspect of the invention therefore there is provided a curing process in which a polymer  
25 having pendent groups of the formulae  $\text{Si}(\text{OR}^{26})_3$ , in which each group  $\text{R}^{26}$  is independently selected from  $\text{C}_{1-4}$ -alkyl, is contacted with gaseous ethylene oxide to provide a cured polymer.

In this aspect of the invention, the silyl group is generally introduced by forming the polymer from ethylenically unsaturated monomers including a  
30 monomer of the formula VIII





VIII


wherein

12

$Y^2$  is selected from



$\text{CH}_2=\text{C}(\text{R}^{23})-\text{CH}_2-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})-\text{CH}_2 \text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})\text{OC}(\text{O})-$ ,  
 $\text{CH}_2=\text{C}(\text{R}^{23})-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})\text{CH}_2\text{OC}(\text{O})\text{N}(\text{R}^{24})-$ ,  $\text{R}^{25}\text{OOC}\text{CR}^{23}=\text{CR}^{23}\text{C}(\text{O})-\text{O}-$ ,  
 $\text{R}^{23}\text{CH}=\text{CHC}(\text{O})\text{O}-$ ,  $\text{R}^{23}\text{CH}=\text{C}(\text{COOR}^{25})\text{CH}_2-\text{C}(\text{O})-\text{O}-$ ,

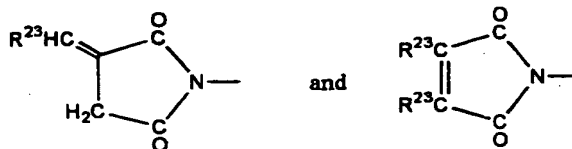

wherein:

$\text{R}^{23}$  is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group;

$\text{R}^{24}$  is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group or  $\text{R}^{24}$  is  $\text{R}^{30} \text{Q}^1$ ;

$\text{R}^{25}$  is hydrogen or a  $\text{C}_{1-4}$  alkyl group;

$\text{A}^7$  is  $-\text{O}-$  or  $-\text{NR}^{24}-$ ; and

$\text{K}^2$  is a group  $-(\text{CH}_2)_t\text{OC}(\text{O})-$ ,  $-(\text{CH}_2)_t\text{C}(\text{O})\text{O}-$ ,

$-(\text{CH}_2)_t\text{OC}(\text{O})\text{O}-$ ,  $-(\text{CH}_2)_t\text{NR}^{28}-$ ,  $-(\text{CH}_2)_t\text{NR}^{28}\text{C}(\text{O})-$ ,

$-(\text{CH}_2)_t\text{C}(\text{O})\text{NR}^{28}$ ,  $-(\text{CH}_2)_t\text{NR}^{28}\text{C}(\text{O})\text{O}-$ ,  $-(\text{CH}_2)_t\text{OC}(\text{O})\text{NR}^{28}-$ ,

$-(\text{CH}_2)_t\text{NR}^{28}\text{C}(\text{O})\text{NR}^{28}-$  (in which the groups  $\text{R}^{28}$  are the same or different),

$-(\text{CH}_2)_t\text{O}-$ ,  $-(\text{CH}_2)_t\text{SO}_3-$ , or a valence bond

$t$  is from 1 to 12;

and  $\text{R}^{28}$  is hydrogen or a  $\text{C}_1-\text{C}_4$  alkyl group;

$\text{R}^{30}$  is a straight or branched  $\text{C}_{2-24}$  alkanediyl group, or a  
 alkyleneoxaalkylene or alkylene(oligo-oxaalkylene) group in which each  
 alkylene has 2 to 12 carbon atoms, and

$\text{Q}^1$  is a group  $\text{Si}(\text{OR}^{26})_3$

the groups  $\text{R}^{26}$  are independently selected from  $\text{C}_{1-4}$  alkyl groups.

Preferably each of the groups  $R^{26}$  are  $C_{1 \text{ or } 2}$ -alkyl, most preferably methyl.

5 In groups  $R^{30}$ , an alkyleneoxealkylene or alkylene(oligo-oxaalkylene) group, has alkylene groups of 2 to 3 carbon atoms, most preferably 2 carbon atoms. Most preferably  $R^{30}$  is an alkanediyl group, most preferably having 2 to 6 carbon atoms, most preferably 3 or 4 carbon atoms. Most preferably it is a group  $(CH_2)_{2 \text{ to } 4}$ -alkyl group.

10 Preferably the polymer is formed from ethylenically unsaturated monomers also including monomer of the formula I described above. The monomers preferably also include a monomer of the formula II above in which the group Q is a crosslinkable group of the formulae  $R^{20} Q$  in which Q is a hydroxyl group.  $R^{20}$  maybe any of the groups defined above for  $R^{30}$ .

15 Ethylene oxide contact is generally conducted under conditions used for sterilization procedures. For instance gas is contacted with the polymer for a period of at least an hour, more preferably at least 2 hours for instance up to 12 hours or even more, at a temperature of at least 40C, more preferably at least 45C up to 70C, most preferably 45-55C, optionally in the presence of steam and usually with a diluent, carrier gas of nitrogen or another inert gas. The proportion in the total gas of ethylene oxide is  
20 preferably at least 50%, more preferably at least about 80%. Treatment may conveniently be carried out under reduce pressure. After treatment the residual ethylene oxide is removed and then the polymer is usually blanketed by nitrogen and washed with air, for instance in several steps.

25 The invention provides also a method of producing the novel kit by coating an assembly consisting of a balloon catheter having a stent mounted on the balloon with a liquid coating composition containing a film forming polymer, and then curing the coating composition.

30 The process is generally carried out by dipping the assembly into a volume of the liquid composition, preferably so that the entire stent is immersed within the volume of liquid. Where only partial coating is required, the assembly maybe dipped to a depth whereby the portion to be desired is immersed in the liquid. Where it is desired to coat discrete areas of the

surface, for instance discrete axially separated rings on the surface, it is convenient for the composition to be applied by spraying.

The liquid coating composition preferably comprises a film forming polymer and a solvent in which the polymer is dissolved or dispersed.

5 Curing generally comprises removal of the solvent, for instance by evaporation under raised temperature and/or reduced pressure.

Curing preferably also comprises crosslinking of a crosslinkable polymer in the coating composition. Crosslinking maybe carried out before, during and/or after solvent removal. Crosslinking of a polymer which  
10 includes crosslinkable groups (as described above) involves subjecting the polymer to conditions under which the crosslinkable groups react to form inter-and intra molecular bonds. Such conditions generally involve heating the polymer, exposing it to incident actinic radiation and/or to moisture or gaseous crosslinking agents. Such agents may include ethylene oxide.

15 Preferably the method includes the step of sterilizing the coated assembly. Sterilization may be carried out simultaneously with curing and/or crosslinking steps. Sterilization may involve subjecting the coated assembly to raised temperature and/or pressure, irradiating the assembly and/or contacting the coated assembly with ethylene oxide. Preferably sterilization  
20 is carried out by contacting the coated assembly with ethylene oxide under the conditions described above in connection with the second aspect of the invention.

Most balloon catheters comprise a guidewire lumen so that the catheter can be run on a pre-positioned guidewire for navigation through the  
25 desired body lumens. In the present invention it may be desirable to coat the inside of the body lumen with the same type of coating as the exterior surface of the stent and balloon. The method therefore it maybe desirable to allow the coating composition to coat the guide wire lumen, for instance by leaving the lumen open during a dipping step and/or by directing liquid  
30 compositions through the lumen during a dipping or spraying process. Alternatively it maybe desired to avoid coating the guidewire lumen, for

instance to avoid reducing the internal diameter of the lumen. In this case, the lumen may be blocked during the coating process using a suitable bung.

In the kit of the invention the coherent coating should have a thickness which avoids increasing the external diameter of the kit by an unacceptable amount, but which has adequate thickness to provide mechanical strength to improve retention of the stent by the desired amount. The thickness should not be so high as increase the pressure at which the balloon deploys the stent. The coating thickness, on the stent external surface, is preferably in the range 5 to 500nm, most preferably in the range 10 to 200nm, for instance in the range 20 to 100nm. The coating may have the same thickness on the balloon and on the stent or may be thicker on the surface of the balloon.

The coating thickness may be adjusted as desired by controlling the rheology of the liquid coating composition, for instance by controlling the concentration, by selecting suitable coating conditions, for instance in terms of temperature, number of coatings of liquid composition applied, or by selecting suitable drying conditions, for instance in terms of the conditions under which excess liquid coating composition is allowed to drain from the stent, as well as conditions of temperature and/or reduced pressure.

In the method, the coating composition preferably has a polymer concentration in the range 2 to 50 g/l, most preferably in the range 5 to 25 g/l, for instance in the range 10 to 20 g/l.

The solvent in the coating composition is, for instance, an alcohol (including glycol), ether, water, alkane or mixtures. Preferably the solvent consists of ethanol, optionally with glycol, mixed with water or with alkane.

The stent is generally formed from a metallic tube provided with openings to confer balloon expandability. Alternatively the stent may be formed from bent or braided wires. Preferred stents have a wall thickness in the range 0.5 to 2.5 mm, most preferably being at least 1000 times the thickness of the coating (average). Preferably the stent is formed from stainless steel. It will often already be provided with an overall coating of biocompatible material. The overall coating may be formed of the same or

different polymer as the polymer in the coating. It suitable has a thickness such that the total polymer coating thickness including the coherent film is less than 500nm thick, for instance less than 250nm thick.

We have found that the provision of a polymer coating on the outside  
5 of the stent/balloon catheter assembly provides improved retention of the stent on the catheter when subjected to axially directed forces, without any deterioration in the ability of the stent to be deployed effectively. The coating does not adversely effect the burst pressures of the balloons, nor the pressures to which the balloons needed to be inflated to achieve stent  
10 deployment. Since the coatings are biocompatible, and indeed have already been approved for use for coating stents for long term implantation, the biocompatibility will not be compromised.

The invention is illustrated further in the following examples.

#### 15        **Example 1**

The polymer used for this example was simplified as described in WO-A-98/30615, polymer 05. The polymer was formed from 2-(methacryloyloxyethyl)-2'-(trimethylammoniumethyl) phosphate inner salt: dodecyl methacrylate: 3-hydroxypropyl methacrylate: 3-trimethoxysilylpropyl  
20 methacrylate in molar ratios of 23:47:25:5. Solutions of the polymer were made up in ethanol at different polymer concentrations. The test assemblies comprised Divysio stents, with (unexpanded outer) diameter 1.6mm, length 28mm and wall thickness 0.914mm, formed of stainless steel and provided with a biocompatible coating comprised of the same polymer as used in this  
25 example on all surfaces at a coating thickness of about 20-100um, mounted on a Nycomed Copan balloon catheter having a 30mm balloon having an expanded diameter (at 6 atm ( $6 \times 10^5$  Pa)) of 3.5mm. The stents were crimped onto the balloons of the balloon catheters using a standard crimping device with jaws of 0.036 in (0.91 mm) at a pressure of 80psi ( $5.5 \times 10^5$  Pa), all  
30 stents being mounted under the same conditions. The guidewire lumen of the balloon catheter was blocked using a suitably sized stylet.

The assembly of stent and balloon catheter was coated by dipping to a depth such that the stent was completely immersed in a volume of coating composition and then withdrawn vertically upwardly at a rate of approximately 1 mm/s. The coated assemblies were dried and cured by heating to 70°C for 4 hours.

The coated assemblies were then subjected to tests to determine the retention of the stent on the balloon and stent deployment. Different samples were used for the different tests.

The retention of the stent onto the balloon was measured by gripping the distal end of the catheter and drawing it through a 1.0mm orifice, which is too small for the stent to pass through. The force is thus exerted in a direction to shift the stent proximally. The retention values are set out in table 1 below, which shows the mean retention for 4 samples coated from different concentrations of polymer as specified, as well as the percentage increase in retention.

**Table 1**

Polymer Concentration (g/l)	Mean Retention (N)	% increase in retention compared to control
Control	2.93	
2.0	2.75	-6.0
6.0	3.78	25.1
8.0	4.53	55.5
10.0	4.71	61.5

### **Example 2**

Assemblies coated as in example 1 with 10 g/l of the same polymer were subjected to tests of their deployment characteristics. The balloon catheter was inflated in 0.5 atmosphere (50 kPa) increments using a

Bundenberg pressure gauge. The results of the individual tests are reported in table 2.

For each of the stents, there was gradual, immediate and even detachment of the stent from the balloon at full deployment. Following deployment there was free movement of the balloon from the stent for each of the samples. In no instances does the balloon burst during deployment.

10

**Table 2**

15

Stent ID	Deployment Pressure (Atm)/Deployment Extent	
1	1.0	a
	1.5	c
	2.0	e
2	1.0	b
	1.5	c
	2.0	e
3	1.0	b
	1.5	c
	2.0	d
	2.5	e
4	1.0	b
	1.5	c
	2.0	d
	2.5	e

5	1.0	a
	1.5	c
	2.0	d
	2.5	e
6	1.0	a
	1.5	c
	2.0	d
	2.5	e

**Key**

- 5      a: no change  
b: slight inflation of the balloon  
c: stent flared, balloon slightly inflated at end  
d: partial inflation of the balloon, and flaring of stent end  
e: immediate (within about 5s) full deployment

10

The coated stents were also characterised for their total coating thickness using atomic force microscopy. This indicated the mean coating thickness for the stent of the kit of the invention is about 80 nm, whilst that of the starting stents is about 50 nm. The extra thickness from the coherent coating used in the invention over the mounted stent is thus believed to be about 30 nm.

15

The specification for the balloon catheter requires that the stent should fully deploy at 8 atmospheres or less. The results taken as a whole indicate that each sample deploys satisfactorily. In combination with the results of example 1, this shows that the overcoating increases retention of the stent without adversely affecting the deployment characteristics.

20

**Example 3**

Further assemblies of stents mounted on balloon catheters were coated using the 10 g/l polymer composition in ethanol, dried and cured

25

using the same conditions as in example 1. In the example the coated assemblies were sterilized using a ethylene oxide sterilization cycle in which a small amount of steam is introduced into the chamber of the sterilizing device followed by a higher amount of ethyleneoxide. The assemblies are maintained in contact with the gas for a period of 5 hours at a pressure of about 350Pa and a temperature of 50C. Following exposure to the gas the gas is removed by evacuating the chamber then the chamber is filled sequentially with nitrogen and then clean volumes of air in several steps.

The retention values were measured using a technique similar to that used in example 1, but in which the stent was subjected to a force to move is distally rather than proximally . The coated assemblies were compared with control, uncoated assemblies.

The results are shown in table 3 below.

**Table 3**

Sample	Retention		
	Mean (n=4)(N)	St.Dev(N)	% increase
Control	1.55	0.19	
Invention	3.68	0.40	137

The results indicate that ethylene oxide treatment following curing leads to a greater increase in stent retention than coating and crosslinking by heating alone.

#### **Example 4**

Further samples of the coated assemblies produced in example 3 were subjected to the deployment test described in example 1. Subsequent to the deployment tests, the balloons were and inflated up to failure. The balloons from the tests of example 3 were also subsequently inflated to failure.

The deployment tests indicate satisfactory deployment very similar to stents 3 to 6 in Example 1. Thus all tested samples were fully deployed at 2.5 atmosphere, within 5 seconds of the imposition of the pressure.

The results of the burst tests are shown in table 4. Samples 4.1 to 4.4 had been subjected to retention tests whilst samples 4.5 and 4.6 had been subjected to deployment tests.

**Table 4**

Sample	Burst Pressure (atm/ $10^5$ Pa)	Failure Mode
4.1	18.0	Pinhole
4.2	20.0	Axial split
4.3	20.0	Axial split
4.4	18.0	Pinhole
4.5	19.7	Axial split
4.6	20.4	Axial split

The "pinhole" failures observed were caused by the piercing of the balloon measurement of the retention values. It is considered unlikely that the pinholes in the balloons were caused by the overcoating. Since it is unlikely that the stent will be subjected to forces as high as those required to dislodge the stent from the balloon during normal use, it is believed that the overcoating of the present invention is unlikely to result in any increase compared to the control of pinhole failures. The average burst pressure of balloons having been used to deploy stents is about 20-22 x  $10^5$  Pa. The coating appears not to reduce this. In any event all pressures recorded at failure were higher than the minimum pressure required in a product specification which is 16 atm ( $10^5$ Pa).

#### **Example 5**

Further sampling of the stent/catheter assembly used in the previous examples were coated with a copolymer of 2-methacryloyloxyethyl-2-

trimethyl ammoniumethyl phosphate inner salt: dodecyl-methacrylate 1:2  
(molar) synthesised substantially as in example 1 of WO-A-9301221) from a  
10 g/l solution in ethanol. The coated assemblies (without prior sterilisation)  
were subjected to the retention test. The retention rates were about 60%  
5 higher than those of the control.

## Claims

1. A kit comprising a balloon catheter comprising a balloon at or near its distal end, and a stent mounted on the balloon, characterized in that in that the exterior surface of the balloon and stent are provided with a coherent  
5 coating comprising a film-forming polymer.
2. A kit according to claim 1 in which the coating is continuous around the circumference of the exterior surface of the balloon and stent over at least a portion of the axial extent of that section.
3. A kit according to claim 1 or claim 2 in which the coating extends  
10 along the entire axial length of the stent, preferably beyond both ends thereof.
4. A kit according to any preceding claim in which the polymer of the coating is cross-linked.
5. A kit according to any preceding claim in which the polymer has  
15 pendent zwitterionic groups.
6. A kit according to claim 5 in which the polymer is formed from ethylenically unsaturated monomers including a zwitterionic monomer of the general formula I:

YBX



I

20 wherein

B is a straight or branched alkylene (alkanediyl), alkyleneoxaalkylene or alkylene oligo-oxaalkylene chain optionally containing one or more fluorine atoms up to and including perfluorinated chains or, if X or Y contains a terminal carbon atom bonded to B, a valence bond;

25 X is a zwitterionic group; and


Y is an ethylenically unsaturated polymerisable group selected from



24

CH<sub>2</sub>=C(R)-CH<sub>2</sub>-O-, CH<sub>2</sub>=C(R)-CH<sub>2</sub>OC(O)-, CH<sub>2</sub>=C(R)OC(O)-, CH<sub>2</sub>=C(R)-O-,  
 CH<sub>2</sub>=C(R)CH<sub>2</sub>OC(O)N(R<sup>1</sup>)-, R<sup>2</sup>OOCCR=CRC(O)-O-, RCH=CHC(O)O-,  
 RCH=C(COOR<sup>2</sup>)CH<sub>2</sub>-C(O)-O-,

5

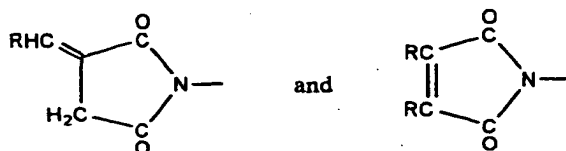

wherein:

R is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group;

10 R<sup>1</sup> is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group or R<sup>1</sup> is -B-X where B and X are as defined above; and

R<sup>2</sup> is hydrogen or a C<sub>1-4</sub> alkyl group;


A is -O- or -NR<sup>1</sup>-;

15 K is a group -(CH<sub>2</sub>)<sub>p</sub>OC(O)-, -(CH<sub>2</sub>)<sub>p</sub>C(O)O-,  
 -(CH<sub>2</sub>)<sub>p</sub>OC(O)O-, -(CH<sub>2</sub>)<sub>p</sub>NR<sup>3</sup>-, -(CH<sub>2</sub>)<sub>p</sub>NR<sup>3</sup>C(O)-,  
 -(CH<sub>2</sub>)<sub>p</sub>C(O)NR<sup>3</sup>-, -(CH<sub>2</sub>)<sub>p</sub>NR<sup>3</sup>C(O)O-, -(CH<sub>2</sub>)<sub>p</sub>OC(O)NR<sup>3</sup>-,  
 -(CH<sub>2</sub>)<sub>p</sub>NR<sup>3</sup>C(O)NR<sup>3</sup>- (in which the groups R<sup>3</sup> are the same or different),  
 -(CH<sub>2</sub>)<sub>p</sub>O-, -(CH<sub>2</sub>)<sub>p</sub>SO<sub>3</sub> -, or, optionally in combination with B, a valence bond  
 p is from 1 to 12; and

20 R<sup>3</sup> is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group.

7. A kit according to claim 6 in which X is a group having the general formula III

25

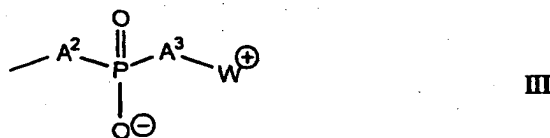

in which the moieties A<sup>2</sup> and A<sup>3</sup>, which are the same or different, are -  
 O-, -S-, -NH- or a valence bond, preferably -O-, and W<sup>+</sup> is a group  
 30 comprising an ammonium, phosphonium or sulphonium cationic group and a  
 group linking the anionic and cationic moieties which is preferably a C<sub>1-12</sub>-  
 alkanediyl group,

preferably in which W<sup>+</sup> is a group of formula

25

$-W^1-N^+R^9_3$ ,  $-W^1-P^+R^{10}_3$ ,  $-W^1-S^+R^{10}_2$  or  $-W^1-Het^+$  in which:


$W^1$  is alkanediyl of 1 or more, preferably 2-6 carbon atoms optionally containing one or more ethylenically unsaturated double or triple bonds, disubstituted-aryl (arylene), alkylene arylene, arylene alkylene, or alkylene aryl alkylene, cycloalkanediyl, alkylene cycloalkyl, cycloalkyl alkylene or alkylene cycloalkyl alkylene, which group  $W^1$  optionally contains one or more fluorine substituents and/or one or more functional groups; and

either the groups  $R^9$  are the same or different and each is hydrogen or alkyl of 1 to 4 carbon atoms, preferably methyl, or aryl, such as phenyl, or two of the groups  $R^9$  together with the nitrogen atom to which they are attached form an aliphatic heterocyclic ring containing from 5 to 7 atoms, or the three groups  $R^9$  together with the nitrogen atom to which they are attached form a fused ring structure containing from 5 to 7 atoms in each ring, and optionally one or more of the groups  $R^9$  is substituted by a hydrophilic functional group, and

the groups  $R^{10}$  are the same or different and each is  $R^9$  or a group  $OR^9$ , where  $R^9$  is as defined above; or

Het is an aromatic nitrogen-, phosphorus- or sulphur-, preferably nitrogen-, containing ring, for example pyridine.

8. A kit according to claims 7 in which X is a group having the general formula IV:

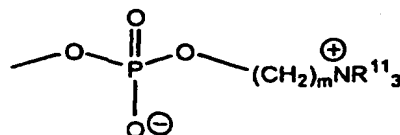

IV

where the groups  $R^{11}$  are the same or different and each is hydrogen or  $C_{1-4}$  alkyl, and m is from 1 to 4, in which preferably the groups  $R^{11}$  are the same preferably methyl.

9. A kit according to any of claims 4 to 9 in which the monomers used to form the polymer include a surface binding monomer having the general formula II



26

 $Y^1R^4$ 

II

wherein  $Y^1$  is selected from


5




10

$CH_2=C(R^5)-CH_2-O-$ ,  $CH_2=C(R^5)-CH_2OC(O)-$ ,  $CH_2=C(R^5)OC(O)-$ ,  $CH_2=C(R^5)-O-$ ,  $CH_2=C(R^5)CH_2OC(O)N(R^6)-$ ,  $R^7OOC-CR^5=CR^5C(O)-O-$ ,  $R^5CH=CHC(O)O-$ ,  $R^5CH=C(COOR^7)CH_2-C(O)-O-$ ,

15



and



wherein:

$R^5$  is hydrogen or a  $C_1-C_4$  alkyl group;

$R^6$  is hydrogen or a  $C_1-C_4$  alkyl group or  $R^6$  is  $R^4$ ;

$R^7$  is hydrogen or a  $C_{1-4}$  alkyl group;

20  $A^1$  is  $-O-$  or  $-NR^6-$ ; and

$K^1$  is a group  $-(CH_2)_qOC(O)-$ ,  $-(CH_2)_qC(O)O-$ ,

$-(CH_2)_qOC(O)O-$ ,  $-(CH_2)_qNR^8-$ ,  $-(CH_2)_qNR^8C(O)-$ ,

$-(CH_2)_qC(O)NR^8-$ ,  $-(CH_2)_qNR^8C(O)O-$ ,  $-(CH_2)_qOC(O)NR^8-$ ,

$-(CH_2)_qNR^8C(O)NR^8-$  (in which the groups  $R^8$  are the same or different),

25  $-(CH_2)_qO-$ ,  $-(CH_2)_qSO_3-$ , or a valence bond

$q$  is from 1 to 12;

and  $R^8$  is hydrogen or a  $C_1-C_4$  alkyl group;

and  $R^4$  is a surface binding group, selected from hydrophobic groups,

ionic groups, reactive groups capable of forming covalent bonds with surface

30 functional groups on the surface of the tube and crosslinkable groups

capable of forming intermolecular crosslinks, optionally in conjunction with

curing agents.

27

10. A kit according to any of claims 4 to 9 in which the polymer is formed from ethylenically unsaturated monomers including a monomer of formula VIII

Y<sup>2</sup>R<sup>30</sup>Q<sup>1</sup>



VIII

5

wherein


Y<sup>2</sup> is selected from

10



CH<sub>2</sub>=C(R<sup>23</sup>)-CH<sub>2</sub>-O-, CH<sub>2</sub>=C(R<sup>23</sup>)-CH<sub>2</sub>OC(O)-, CH<sub>2</sub>=C(R<sup>23</sup>)OC(O)-,  
 CH<sub>2</sub>=C(R<sup>23</sup>)-O-, CH<sub>2</sub>=C(R<sup>23</sup>)CH<sub>2</sub>OC(O)N(R<sup>24</sup>)-, R<sup>25</sup>OOCCR<sup>23</sup>=CR<sup>23</sup>C(O)-O-,  
 R<sup>23</sup>CH=CHC(O)O-, R<sup>23</sup>CH=C(COOR<sup>25</sup>)CH<sub>2</sub>-C(O)-O-,

15

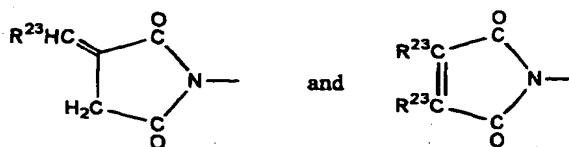

wherein:

20

R<sup>23</sup> is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group;R<sup>24</sup> is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group or R<sup>24</sup> is R<sup>30</sup>Q<sup>1</sup>;R<sup>25</sup> is hydrogen or a C<sub>1-4</sub> alkyl group;A<sup>7</sup> is -O- or -NR<sup>24</sup>-; andK<sup>2</sup> is a group -(CH<sub>2</sub>)<sub>t</sub>OC(O)-, -(CH<sub>2</sub>)<sub>t</sub>C(O)O-,

25

-(CH<sub>2</sub>)<sub>t</sub>OC(O)O-, -(CH<sub>2</sub>)<sub>t</sub>NR<sup>28</sup>-, -(CH<sub>2</sub>)<sub>t</sub>NR<sup>28</sup>C(O)-,-(CH<sub>2</sub>)<sub>t</sub>C(O)NR<sup>28</sup>-, -(CH<sub>2</sub>)<sub>t</sub>NR<sup>28</sup>C(O)O-, -(CH<sub>2</sub>)<sub>t</sub>OC(O)NR<sup>28</sup>-,-(CH<sub>2</sub>)<sub>t</sub>NR<sup>28</sup>C(O)NR<sup>28</sup>- (in which the groups R<sup>28</sup> are the same or different),-(CH<sub>2</sub>)<sub>t</sub>O-, -(CH<sub>2</sub>)<sub>t</sub>SO<sub>3</sub> -, or a valence bond

t is from 1 to 12;


30

and R<sup>28</sup> is hydrogen or a C<sub>1</sub>-C<sub>4</sub> alkyl group;

$R^{30}$  is a straight or branched  $C_{2-24}$  alkanediyl group, or a alkylenoxaalkylene or alkylene(oligo-oxaalkylene) group in which each alkylene has 2 to 12 carbon atoms, and

$Q^1$  is a group  $Si(OR^{26})_3$  in which the groups  $R^{26}$  are independently  
5 selected from  $C_{1-4}$  alkyl groups.

11. A kit according to claim 10 in which  $Y^2$  is



10 in which  $R^{23}$  is preferably methyl, and  $A^7$  is preferably  $-O-$ , and in which  $R^{30}$  is  $C_{2-6}$  alkanediyl and each  $R^{26}$  is  $C_{1-2}$ -alkyl, preferably methyl.

12. A kit according to any preceding claim which is sterile, preferably sterilised by ethylene oxide treatment.

13. A kit according to any preceding claim in which the luminal surface of  
15 the guidewire lumen has not been provided with the said coherent coating.

14. A kit according to any preceding claim in which the stent is formed from a metal tube, preferably of stainless steel.

15. A method in which an assembly comprising a balloon catheter and, mounted on the balloon of the balloon catheter, a stent is coated with a  
20 liquid coating composition containing a film-forming polymer, and the coating composition is then cured to leave a coherent film of polymer on the exterior surface of the stent and balloon.

16. A method according to claim 15 in which in the coating step the balloon and stent assembly is dipped into the liquid composition.

25 17. A method according to claim 16 in which the catheter has a guidewire lumen passing through the balloon and the lumen is blocked during the dipping step.

18. A method according to any of claims 15 to 17 in which curing involves removal of solvent from the coating composition, preferably by evaporation.

19. A method according to claim 18 in which the solvent in the coating composition comprises water, alcohol, ether, or alkane or mixtures, preferably ethanol in admixture with water or alkane.

20. A method according to any of claims 15 to 19 in which the film-forming polymer is cross-linkable and the curing step includes a step of cross-linking the polymer.

21. A method according to claim 20 in which the polymer is as defined in claim 10 or claim 11.

22. A method according to any of claims 15 to 21 in which the coated assembly is sterilised by contact with ethylene oxide.

23. A curing process in which a polymer having pendent groups of the formula  $\text{Si}(\text{OR}^{26})_3$ , in which each group  $\text{R}^{26}$  is independently selected from  $\text{C}_{1-4}$ -alkyl, is contacted with gaseous ethylene oxide to provide a cured polymer.



24. A curing process according to claim 23 in which the silyl group is introduced into the polymer by forming the polymer from ethylenically unsaturated monomers including a monomer of the formula VIII




VIII

wherein


$\text{Y}^2$  is selected from



$\text{CH}_2=\text{C}(\text{R}^{23})-\text{CH}_2-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})-\text{CH}_2 \text{OC}(\text{O})-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})\text{OC}(\text{O})-$ ,  
 $\text{CH}_2=\text{C}(\text{R}^{23})-\text{O}-$ ,  $\text{CH}_2=\text{C}(\text{R}^{23})\text{CH}_2\text{OC}(\text{O})\text{N}(\text{R}^{24})-$ ,  $\text{R}^{25}\text{OOC}\text{CR}^{23}=\text{CR}^{23}\text{C}(\text{O})-\text{O}-$ ,  
 $\text{R}^{23}\text{CH}=\text{CHC}(\text{O})\text{O}-$ ,  $\text{R}^{23}\text{CH}=\text{C}(\text{COOR}^{25})\text{CH}_2-\text{C}(\text{O})-\text{O}-$ ,



and



wherein:

$R^{23}$  is hydrogen or a  $C_1$ - $C_4$  alkyl group;

$R^{24}$  is hydrogen or a  $C_1$ - $C_4$  alkyl group or  $R^{24}$  is  $R^{30} Q^1$ ;

$R^{25}$  is hydrogen or a  $C_{1-4}$  alkyl group;

5  $A^7$  is  $-O-$  or  $-NR^{24}-$ ; and

$K^2$  is a group  $-(CH_2)_t OC(O)-$ ,  $-(CH_2)_t C(O)O-$ ,

$-(CH_2)_t OC(O)O-$ ,  $-(CH_2)_t NR^{28}-$ ,  $-(CH_2)_t NR^{28}C(O)-$ ,

$-(CH_2)_t C(O)NR^{28}$ ,  $-(CH_2)_t NR^{28}C(O)O-$ ,  $-(CH_2)_t OC(O)NR^{28}-$ ,

$-(CH_2)_t NR^{28}C(O)NR^{28}-$  (in which the groups  $R^{28}$  are the same or different),

10  $-(CH_2)_t O-$ ,  $-(CH_2)_t SO_3-$ , or a valence bond

$t$  is from 1 to 12;


and  $R^{28}$  is hydrogen or a  $C_1$ - $C_4$  alkyl group;

$R^{30}$  is a straight or branched  $C_{2-24}$  alkanediyl group, or a  
alkylenoxaalkylene or alkylene(oligo-oxaalkylene) group in which each  
15 alkylene has 2 to 12 carbon atoms, and

$Q^1$  is a group  $Si(OR^{26})_3$  in which the groups  $R^{26}$  are independently  
selected from  $C_{1-4}$  alkyl groups.

25. A curing process according to claim 24 in which in which  $Y^2$  is

20



in which  $R^{23}$  is preferably methyl, and  $A^7$  is preferably  $-O-$ , and in which  $R^{30}$  is  
 $C_{2-6}$  alkanediyl and each  $R^{26}$  is  $C_{1-2}$ -alkyl, preferably methyl.

26. A curing process according to claim 23 or 24 in which the polymer is  
25 as defined in any of claims 5 to 9.

27. A curing process according to any of claims 23 to 26 in which  
ethylene oxide contact is by impinging a gas comprising at least 50%  
ethylene oxide, optionally in combination with steam, on the surface which is  
at a temperature of 45 to 55 C for a period of at least 2 hours preferably at  
30 least 4 hours.

**Abstract****Balloon Expandable Stent**

The present invention relates to a balloon expandable stent mounted  
5 on a balloon catheter, the entire assembly being overcoated with a coherent  
polymer coating, which is preferably substantially continuous over the  
circumference and, more preferably, axial length of the stent on the balloon.  
The polymer coating improves retention of the stent on the balloon during  
delivery and does not adversely effect the deployment characteristics, nor  
10 the balloon failure characteristics. The product is made by mounting the  
stent on the balloon and coating the assembly with a liquid coating  
composition containing a suitable polymer followed by curing of the coating.  
The polymer is biocompatible and preferably crosslinkable in the coating  
composition, and crosslinked in the final product. A suitable polymer is  
15 formed from monomers including a phosphoryl choline group, and monomers  
including a trialkoxysilyl group. Preferably the coated product is contacted  
with ethylene oxide to provide simultaneous sterilization and additional  
curing.

**THIS PAGE BLANK (USPTO)**

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☒ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☒ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☒ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☒ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**

**THIS PAGE BLANK (USPTO)**